
**User's Manual**

# InfraRed Thermometer
**with Laser Pointer**

## MODEL 42529

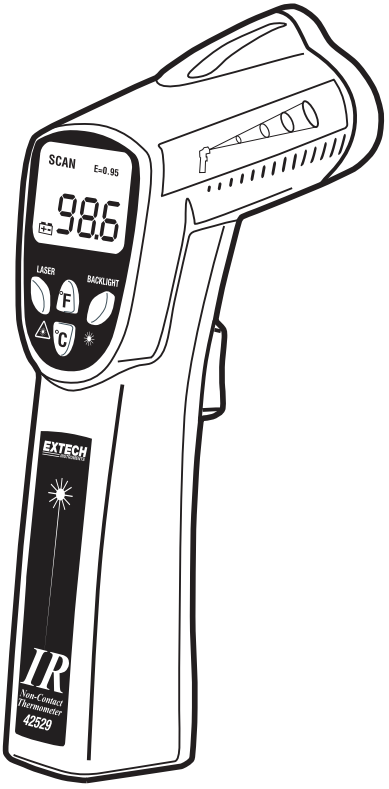


### *Introduction*

Congratulations on your purchase of the Model 42529 IR Thermometer. This thermometer makes non-contact (infrared) temperature measurements at the touch of a button. The built-in laser pointer increases target accuracy while the backlit LCD and handy push-buttons combine for convenient, ergonomic operation. Proper use and care of this meter will provide years of reliable service.

## *Warranty*

EXTECH INSTRUMENTS CORPORATION warrants this instrument to be free of defects in parts and workmanship for three (3) years from date of shipment (a six month limited warranty applies on sensors and cables). If it should become necessary to return the instrument for service during or beyond the warranty period, contact the Customer Service Department at (781) 890-7440 ext. 210 for authorization or visit our website at www.extech.com (click on 'Contact Extech' and go to 'Service Department' to request an RA number). A Return Authorization (RA) number must be issued before any product is returned to Extech. The sender is responsible for shipping charges, freight, insurance and proper packaging to prevent damage in transit. This warranty does not apply to defects resulting from action of the user such as misuse, improper wiring, operation outside of specification, improper maintenance or repair, or unauthorized modification. Extech specifically disclaims any implied warranties or merchantability or fitness for a specific purpose and will not be liable for any direct, indirect, incidental or consequential damages. Extech's total liability is limited to repair or replacement of the product. The warranty set forth above is inclusive and no other warranty, whether written or oral, is expressed or implied.

## *Safety*

- Use extreme caution when the laser pointer beam is on
- Do not point the beam toward anyone's eye or allow the beam to strike the eye from a reflective surface
- Do not use the laser near explosive gases or in other potentially explosive areas




## *Specifications*

**Infrared Thermometer Specifications**


| | | |
|---|---|---|
| Range / Resolution | 0 to 600°F (-20 to 320°C) | 1°C/F |
| Accuracy | ± 2% of reading or ± 4°F (2°C) whichever is greater.<br>Note: Accuracy is specified for the following ambient temperature range: 64 to 82°F (18 to 28°C) | |
| Emissivity | 0.95 fixed value | |
| Field of View | D/S = Approx. 6:1 ratio (D = distance, S = spot) | |
| Laser power | Less than 1mW | |
| Spectral response | 6 to 14 μm (wavelength) | |

**General Specifications**

| | |
|---|---|
| Display | 3½ digit backlit LCD display with function indicators |
| Display rate | 1 second approx. |
| Over range indication | Audible tone sounds and 'OVER' appears on the LCD when the measurement exceeds the measurement range spec. |
| Operating Temperature | 32°F to 122°F (0°C to 50°C) |
| Operating Humidity | Max. 80% RH. |
| Power Supply | 9V battery |
| Automatic Power Off | Meter shuts off automatically after 7 seconds |
| Weight | 6.35 oz. / 180g |
| Size | 8.3 x 3.5 x 1.5" (211 x 89 x 38mm) |

## *Meter Description*

1. LCD Display
2. Function Buttons
3. Handle Grip
4. Laser Pointer
5. IR Sensor
6. Measurement Trigger
7. Battery Compartment

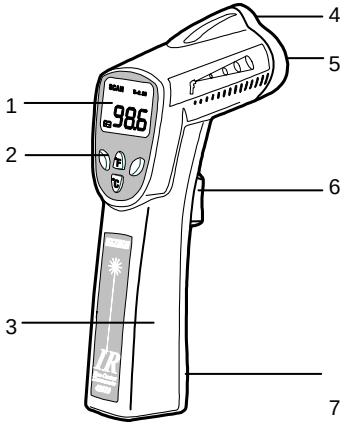



## *Operating Instructions*

1. Hold the meter by its **Handle Grip** and point it toward the device whose temperature is to be measured.
2. Press and hold the red **Trigger** to turn the meter on and begin testing. The display will light if the battery is charged. Replace the battery if the display does not light.
3. While continuing to press the Trigger, push the red **Laser** button to turn on the laser pointer. Aim the red beam approximately a half inch higher than the point of test as shown in the diagram below (pressing the Laser button again turns the laser off).
4. While measuring, the SCAN display icon will appear on the LCD above the temperature measurement and to the left of the emissivity value (fixed at 0.95.).
5. If the measurement exceeds the useable temperature range (0 to 600°F), the meter will emit a tone and the LCD will display 'OVER'.
6. Release the Trigger when the temperature stabilizes. The HOLD display icon will appear on the LCD indicating that the reading is being held.
7. Set the temperature units (°C or °F) using the blue **°C** and **°F** buttons.
8. Press the yellow **Backlight** key to turn on the LCD backlighting function.
9. The meter will automatically power down after 7 seconds.

## *Field of View*

The meter's field of view is 6:1, meaning that if the meter is 6 inches from the target, the diameter of the object under test must be at least 1 inch. Other distances are shown below in the field of view diagram. Refer to the chart printed on the meter for more information.

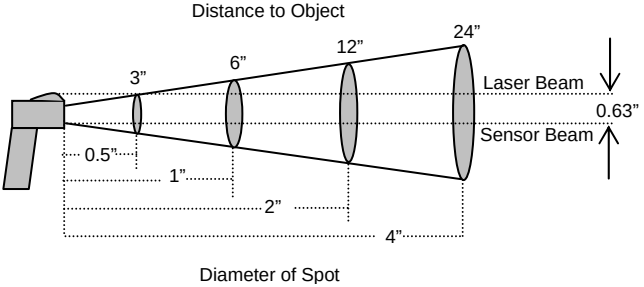

## *Measurement Notes*

1. The object under test should be larger than the spot (target) size calculated by the field of view diagram (see diagram on previous page or on side of the meter).
2. If the surface of the object under test is covered with frost, oil, grime, etc., clean before taking measurements.
3. If an object's surface is highly reflective apply masking tape or flat black paint before measuring.
4. The meter cannot measure through transparent surfaces such as glass.
5. Steam, dust, smoke, etc. can obscure accurate measurements.
6. The meter compensates for deviations in ambient temperature. It can, however, take up to 30 minutes for the meter to adjust to extremely wide ambient temperature changes.
7. To find a hot spot, aim the meter outside the area of interest then scan across (in an up and down motion) until the hot spot is located.

## *Battery Replacement*

When the low battery symbol appears on the LCD, replace the meter's 9V battery. The battery compartment is located on the bottom of the meter's handle. Open the compartment by sliding the battery compartment cover off in the direction of the arrow. Replace battery and re-install the battery compartment cover.

## *Calibration and Repair Services*

**Extech offers repair and calibration services** for the products we sell. Extech also provides NIST certification for most products. Call the Customer Service Department for information on calibration services available for this product. Extech recommends that annual calibrations be performed to verify meter performance and accuracy.


**Support line (781) 890-7440**

Technical support: Extension 200; E-mail: support@extech.com

Repair & Returns: Extension 210; E-mail: repair@extech.com


**Product specifications subject to change without notice**

For the latest version of this User's Guide, Software updates, and other up-to-the-minute product information, visit our website: www.extech.com


Extech Instruments Corporation, 285 Bear Hill Rd., Waltham, MA 02451



**Copyright © 2005 Extech Instruments Corporation**

All rights reserved including the right of reproduction in whole or in part in any form.